


ASAP G1 Instrument

- ▶ Nucleic acid testing using OME developed fluoro-detection technology
- ▶ Accurate results in 20 minutes, fastest in the market
- ▶ Competitive price at less than 10% of regular equipment and reagents
- ▶ High compatibility and applications
- ▶ High connectivity up to 256 units
- ▶ 800g only, compact and portable
- ▶ ISO 13485 and ISO 61010 compliance




Fields of Application and Related Diseases

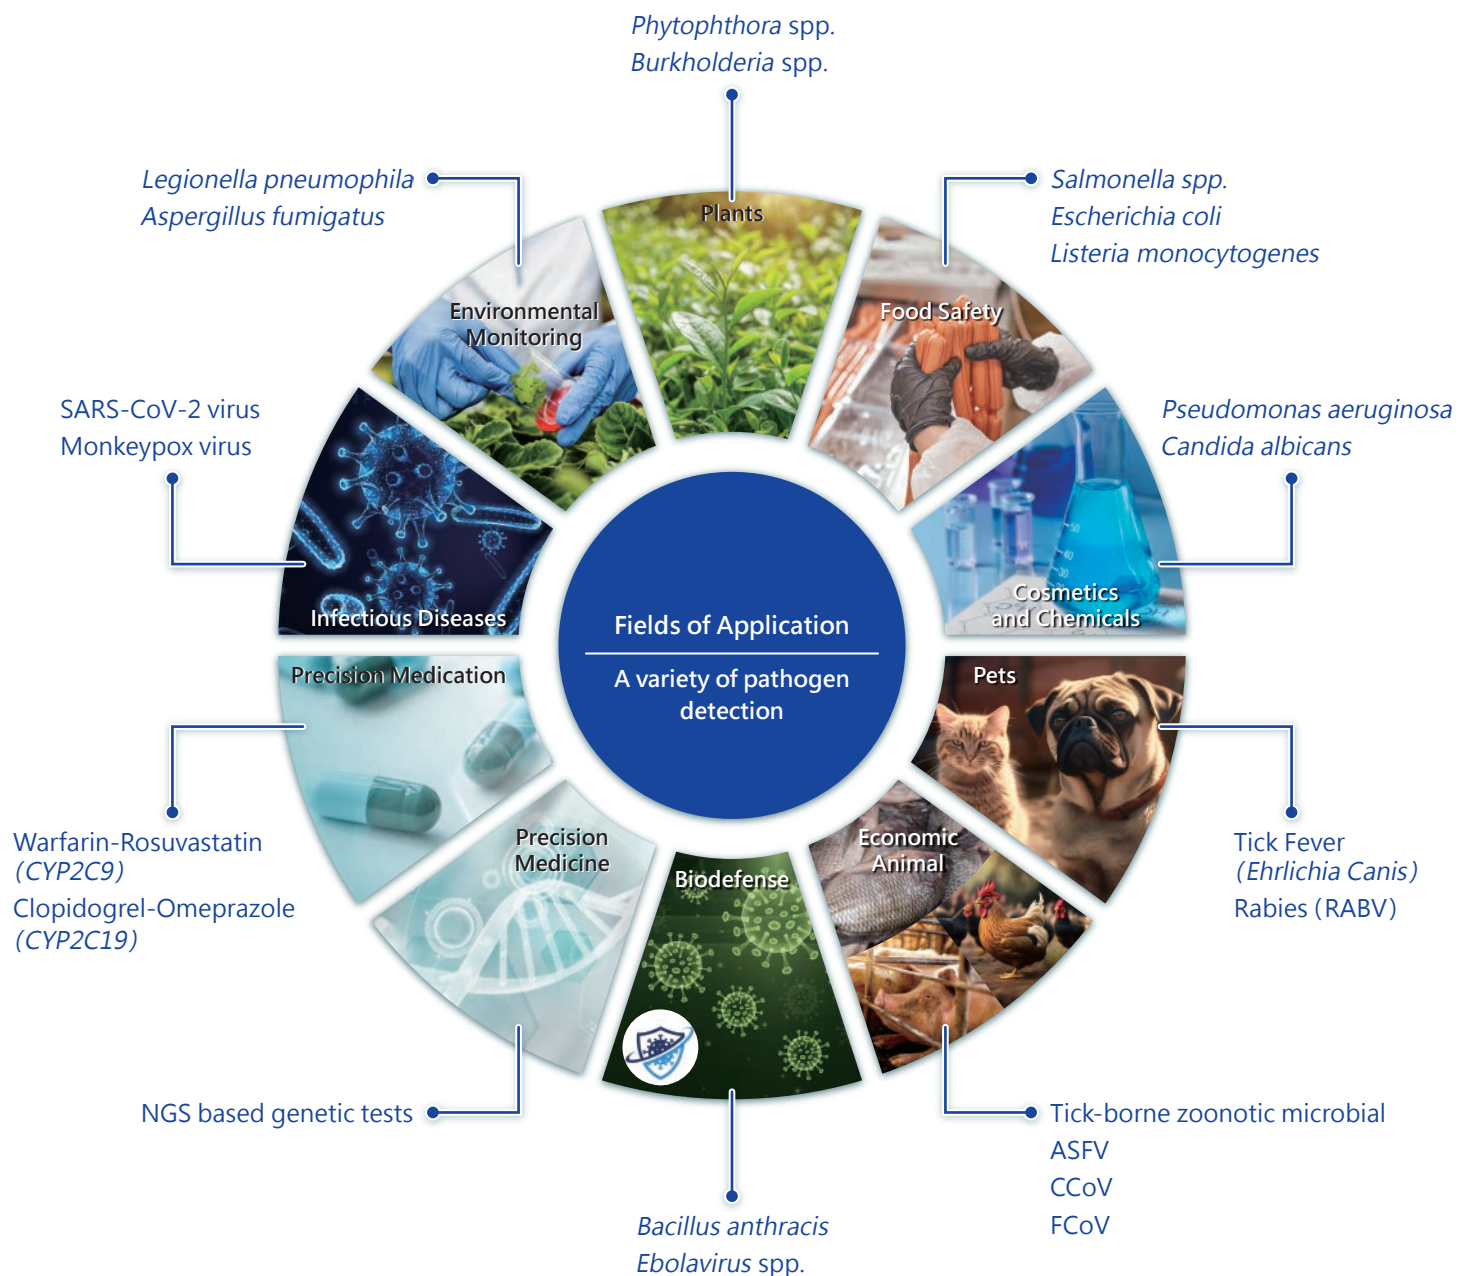


Protocol for Microbial Detection Test


1

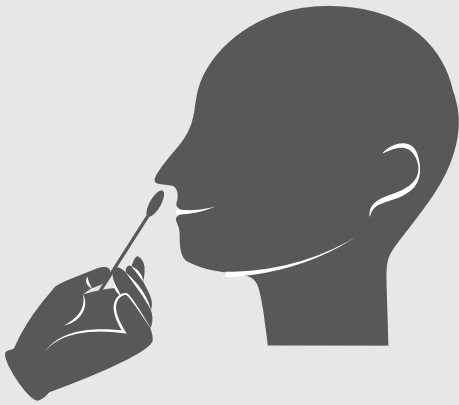


2

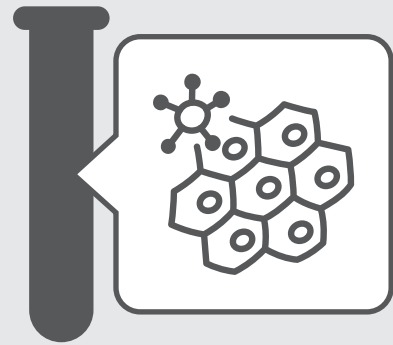

3

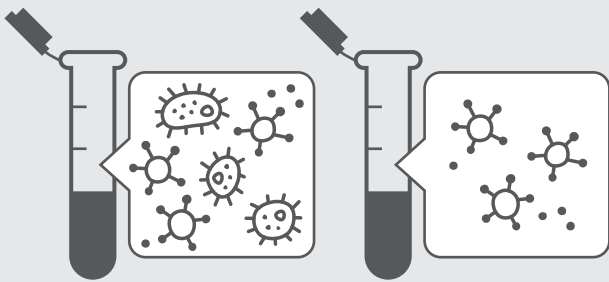

4

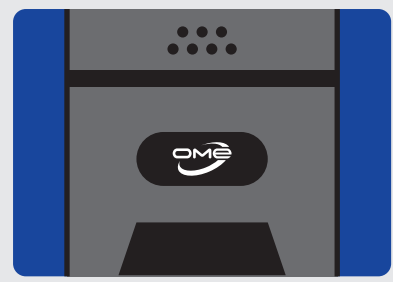

5




6



Operation

High Scalability and Connectivity

The high connectivity, up to 256 units, can be controlled by a laptop or smartphone.

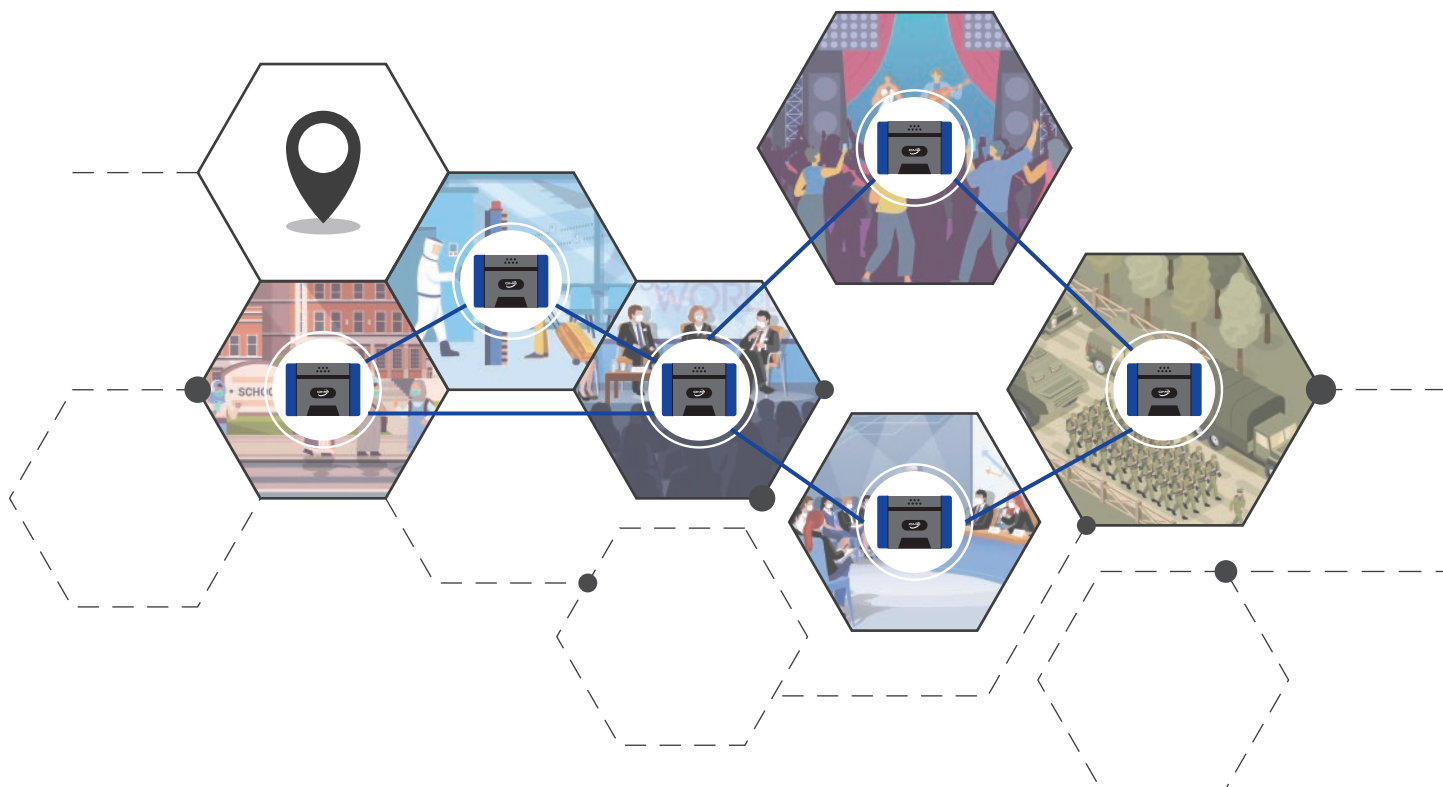

Harmonized International Standards

Industrial Field	Harmonized Standards
Medical Device	ISO 13485 : 2016
	ISO 14971 : 2019
	IEC 61010-1 : 2010+A1 : 2016
	IEC 61010-2-101 : 2018
EMC	EN IEC 61326-1 : 2020
	EN IEC 61326-2-6 : 2020
	EN IEC 61000-3-2 : 2019+A1 : 202
	IEC 61000-4-2 : 2008
	IEC 61000-4-3 : 2020
	IEC 61000-4-4 : 2012 RLV
	IEC 61000-4-5 : 2014+A1 : 2017
	IEC 61000-4-6 : 2013+COR1 : 2015
	IEC 61000-4-8 : 2009
	IEC 61000-4-11 : 2020+COR1 : 2015
Radio Interference	CISPR 11 : 2015+AMD1 : 2016+AMD2 : 2019

